

# Accuracy of impedance cardiography for evaluating trends in cardiac output: a comparison with oesophageal Doppler

E. Lorne<sup>1,3\*</sup>, Y. Mahjoub<sup>1,3</sup>, M. Diouf<sup>2</sup>, J. Slegthem<sup>1</sup>, C. Buchalet<sup>1</sup>, P.-G. Guinot<sup>1</sup>, S. Petiot<sup>1</sup>, A. Kessavane<sup>1</sup>, B. Dehedin<sup>1</sup> and H. Dupont<sup>1,3</sup>

<sup>1</sup> Department of Anesthesiology and Critical Care Medicine and <sup>2</sup> Biostatistics Department, Amiens University Medical Center, Amiens, France

<sup>3</sup> INSERM U1088, Jules Verne University of Picardy, Amiens, France

\* Corresponding author. E-mail: lorne.emmanuel@chu-amiens.fr

## Editor's key points

- Impedance cardiography (ICG) was compared with oesophageal Doppler monitoring (ODM) in determining cardiac output (CO) in general surgery patients.
- In a modified polar plot analysis, CO variations correlated significantly between the two methods.
- ICG is a reliable non-invasive method comparable with ODM in investigating CO trends in general surgical patients.

**Background.** Impedance cardiography (ICG) enables continuous, beat-by-beat, non-invasive, operator-independent, and inexpensive cardiac output (CO) monitoring. We compared CO values and variations obtained by ICG (Niccomo™, Medis) and oesophageal Doppler monitoring (ODM) (CardioQ™, Deltex Medical) in surgical patients.

**Methods.** This prospective, observational, single-centre study included 32 subjects undergoing surgery with general anaesthesia. CO was measured simultaneously with ICG and ODM before and after events likely to modify CO (vasopressor administration and volume expansion). One hundred and twenty pairs of CO measurements and 94 pairs of CO variation measurements were recorded.

**Results.** The CO variations measured by ICG correlated with those measured by ODM [ $r=0.88$  (0.82–0.94),  $P<0.001$ ]. Trending ability was good for a four-quadrant plot analysis with exclusion of the central zone (<10%) [95% confidence interval (CI) for concordance (0.86; 1.00)]. Moderate to good trending ability was observed with a polar plot analysis (angular bias:  $-7.2^\circ$ ; 95% CI  $-12.3^\circ$ ;  $-2.5^\circ$ ; with radial limits of agreement  $-38^\circ$ ;  $24^\circ$ ). After excluding subjects with chronic obstructive pulmonary disease, a Bland–Altman plot showed a mean bias of 0.47 litre  $\text{min}^{-1}$ , limits of agreements between  $-1.24$  and 2.11 litre  $\text{min}^{-1}$ , and a percentage error of 35%.

**Conclusion.** ICG appears to be a reliable method for the non-invasive monitoring of CO in patients undergoing general surgery.

**Keywords:** monitoring; cardiopulmonary, monitoring; ultrasound

Accepted for publication: 10 February 2014

Recent studies have shown that cardiac output (CO) monitoring in the operating theatre reduces morbidity and shortens length of hospital stay after surgery.<sup>1–6</sup> In these studies, the goal was to maintain oxygen delivery and avoid oxygen debt. Anaesthesiologists need less invasive ways of continuously monitoring CO. There is now sufficient evidence to support the use of oesophageal Doppler monitoring (ODM) for routine cardiac monitoring.<sup>7</sup> Thoracic impedance cardiography (ICG) is a non-invasive, continuous, operator-independent, and cost-effective tool for CO monitoring.<sup>8</sup> While some studies have found good agreement between impedance and a reference technique, others have found high limits of agreements reflecting a lack of interchangeability between the ICG and reference techniques.<sup>9</sup> Poor reliability could be because of a poor signal-to-noise ratio, strict requirements for lead placement that make ICG incompatible with certain types of surgery,<sup>10 11</sup> and lack of accuracy in determining left ventricular ejection time (LVET).<sup>12</sup> Bioreactance has been used to overcome these

difficulties. Bioreactance measures the frequency modulation and signal phase shift of an electrical current crossing the thorax, the variations of which are related to changes in the volume of the thoracic aorta.<sup>13</sup> This technology significantly enhances the signal-to-noise ratio.<sup>13</sup> Nevertheless, conflicting results have been found with bioreactance in the clinical context.<sup>14–17</sup>

Recently, the manufacturer of the Niccomo™ ICG monitor (Medis Medizinische Messtechnik GmbH, Ilmenau, Germany) developed a new algorithm and new signal measurement hardware, so that aortic opening and closure could be detected more accurately. By definition, thoracic impedance ( $Z=R+jX$ ) measures the added vector between resistance ( $R$ ) and phase shifted reactance ( $jX$ ) that is the result of capacitance and inductance.<sup>18</sup> Therefore, thoracic impedance variations measure the impedance variations induced by stroke volume (SV)<sup>8</sup> to the resistance and the reactance of the thorax. According to the manufacturer, the new design provides greater

sensitivity and a higher signal-to-noise ratio, so that even very small impedance signals (and thus, blood volume variations) can be reliably detected. On this basis, it is possible to reduce the overall low pass filtering of the signal, which yields a much more information-rich ICG waveform and provides a clearer depiction of the fiducial points required for the calculation of the SV. Furthermore, the system's algorithms for artifact elimination and detection of the fiducial points have been optimized. The new algorithm should allow better acquisition of the X point corresponding to aortic valve closure.<sup>19</sup> Recognition of each heart beat on the electrocardiogram (ECG) and determination of the exact times of aortic opening and closure might also improve the accuracy of the Niccomo™ monitor. In the present study, we compared the ability of ICG and that of ODM to evaluate absolute CO values and CO trends.

## Methods

### Ethical aspects

The study's objectives and procedures were approved by the local institutional review board (*Comité de protection des personnes Nord-Ouest II*, Amiens, France). Written informed consent was waived because the board considered that the study procedures were part of routine practice.

### Subjects

A prospective, observational study was conducted over a 2-month period (February and March 2012) in the Department of Anesthesiology at Amiens University Medical Center (Amiens, France). The inclusion criterion was age  $\geq 18$  yr, with use of ODM during surgery. Patients with preoperative arrhythmia, history of right or left ventricular failure, valvular aortic disease, frequent ectopic beats or spontaneous breathing or contraindications to ODM probe insertion were excluded.

### Anaesthesia

Monitoring consisted of three-lead ECG, pulse oximetry, and non-invasive arterial pressure monitoring. Balanced general anaesthesia was used in all the subjects. Induction was performed with propofol or etomidate and either remifentanyl or sufentanyl, according to the anaesthesiologist's preference. All the patients received neuromuscular block with i.v. cisatracurium ( $0.15 \text{ mg kg}^{-1}$ ) or rocuronium ( $0.6 \text{ mg kg}^{-1}$ ). Tracheal intubation with a single lumen tracheal tube was performed to obtain airway control with mechanical ventilation in the volume-controlled mode. Tidal volume (VT) was  $8\text{--}9 \text{ ml kg}^{-1}$  of ideal body weight (IBW), with ventilatory frequency adjusted to maintain end-tidal  $\text{CO}_2$  concentrations of  $4.0\text{--}4.66 \text{ kPa}$  and a positive end-expiratory pressure (PEEP) of  $3\text{--}5 \text{ cm H}_2\text{O}$ . Anaesthesia was maintained with either propofol or inhaled desflurane or sevoflurane.

### Measurements

Clinical data [age, gender, weight, height, body mass index (BMI), type of surgery, ASA physical status, Lee score, history of heart failure, hypertension, peripheral arterial disease,

coronary syndrome, stroke, chronic kidney disease, diabetes chronic obstructive pulmonary disease (COPD), and smoking status] and ventilatory data (tidal volume, plateau pressure, and end-expiratory pressure) were recorded at baseline.

The CO derived from ODM ( $\text{CO}_{\text{ODM}}$ ) or ICG ( $\text{CO}_{\text{ICG}}$ ) and haemodynamic data were recorded before and after treatments likely to modify CO (vasopressor administration or volume expansion). The indications for these interventions were left to the anaesthetist's discretion. Subjects were studied after 5 min with stable haemodynamic variables, constant ventilator settings, and stable drug administration. A first set of measurements [heart rate (HR), systolic arterial pressure (SAP), mean arterial pressure (MAP), diastolic arterial pressure (DAP),  $\text{SV}_{\text{ODM}}$ ,  $\text{CO}_{\text{ODM}}$ , flow time corrected (FTc), peak velocity (PV),  $\text{SV}_{\text{ICG}}$ , and  $\text{CO}_{\text{ICG}}$ ] was recorded at baseline. Possible treatments were volume expansion (infusion of 500 ml crystalloid solution over 10 min), bolus of phenylephrine ( $50\text{--}100 \mu\text{g}$ ), or norepinephrine infusion ( $0.03\text{--}0.15 \mu\text{g kg}^{-1} \text{ min}^{-1}$ ). A second set of measurements (HR, SAP, MAP, DAP,  $\text{SV}_{\text{ODM}}$ ,  $\text{CO}_{\text{ODM}}$ , FTc, PV,  $\text{SV}_{\text{ICG}}$ , and  $\text{CO}_{\text{ICG}}$ ) was recorded at the end of the treatment (after 5 min of haemodynamic stability).

### Oesophageal Doppler monitoring

The position of the ODM probe (CardioQ™, Deltex Medical, Gamida, Eaubonne, France) was adjusted to obtain the best signal for descending aortic blood velocity.<sup>20</sup> Given that aortic wall motion is possible, we sought to avoid the occurrence of non-laminar flow by narrowing the frequency range (blunt velocity profile). The narrow frequency range has a characteristic shape, with bright borders and dark inner part. The probe was systematically repositioned before each measurement, as recommended.<sup>20</sup> On the basis of continuous aortic blood flow measurements, the acquisition software automatically calculated the SV average over 30 s. The inter-observer variability of the method is good and ranges between 3 and 10%.<sup>21</sup> The reproducibility of SV measurement was tested before the study; SV was measured twice in 10 patients by the same observer and by a second observer in two studies of our group:<sup>22 23</sup> intra-observer reproducibility was 0.3 and 0.5% ( $0.1\text{--}4.0\%$ ) and inter-observer reproducibility was between 1.1 and 2% ( $3\text{--}5\%$ ). CO, SV, FTc, and PV were recorded continuously (beat by beat) from aortic blood velocity, and their mean values were calculated over 30 s using the Excel® file generated by the CardioQ™.

### ICG monitoring

Four Niccomo™ dual-electrode patches (i.e. eight electrodes in all) were placed as recommended by the manufacturer. Current intensity and frequency were 1.5 mA and 85 kHz. The ICG signal is the first derivative of the thoracic impedance ( $Z_0$ ),  $dZ/dt$ , and ejection time into account, the software calculates the SV using Bernstein's equation<sup>8</sup> excluding distortions or artifacts in the ICG signal. The SV was calculated beat by beat and averaged over 30-s periods.

### Statistical analysis

Sample size was calculated in order to demonstrate equivalence between  $\Delta\text{CO}_{\text{ODM}}$  and  $\Delta\text{CO}_{\text{ICG}}$ . With a two-sided alpha risk of 0.05, a beta risk of 0.2, a Pearson correlation between  $\Delta\text{CO}_{\text{ODM}}$  and  $\Delta\text{CO}_{\text{ICG}}$  of 0.8, and an expected *SD* of 0.9 for  $\Delta\text{CO}$ , 31 pairs of  $\Delta\text{CO}$  measurements were needed to demonstrate equivalence with a margin of 0.3 (in a paired test). Given that the  $\Delta\text{CO}$  measurements were repeated an average of three times per subject, the variance inflation factor<sup>24</sup> was estimated to be 1.6 for an intra-class correlation coefficient of 0.3. The adjusted minimum sample size (i.e. the number of pairs of  $\Delta\text{CO}$  measurements) was therefore 50.

The normality of quantitative data was verified using the Kolmogorov–Smirnov test, and data are expressed as mean (*SD*).

The relationship between  $\text{CO}_{\text{ODM}}$  and  $\text{CO}_{\text{ICG}}$  was analysed using a linear, mixed-effects model. Agreement between  $\text{CO}_{\text{ODM}}$  and  $\text{CO}_{\text{ICG}}$  was analysed with scatter plots and Bland–Altman plots. Percentage error was calculated as 1.96 *SD* of the bias divided by mean CO; this value was considered clinically acceptable if <30%. The influence of the population's characteristics on the bias was systematically screened with a Wilcoxon test.

Given that the radial limits of agreement (RLA) approach assumes that each data pair is independent,<sup>25</sup> it is not valid for repeated measures. Accordingly, we developed a polar plot method for repeated measures. Trending ability was studied with two different methods: a four-quadrant plot and a polar plot. We calculated the concordance rate (in the four-quadrant plot only), the angular bias and its *SD*, and the RLA (in the polar plot only).<sup>25</sup> A detailed description of the polar plot method for repeated measures is provided as an appendix. Data at the centre of the polar plot correspond to small changes in CO; the associated, large, random error (statistical noise) component makes it difficult to assess trending.<sup>26</sup> Hence, receiver operating characteristic curves were drawn to make judgements about the discriminative power of different  $\Delta\text{CO}$  values. An optimal  $\Delta\text{CO}$  exclusion value of 10% (mean CO: 4.91 litre  $\text{min}^{-1}$ , hence 10%=0.5 litre  $\text{min}^{-1}$ ) was found. Our exclusion zone limits reflect those commonly used in concordance analysis.<sup>26</sup>


## Results

In the 2-month study period, 36 subjects were enrolled. Four of these were subsequently excluded because of frequent ectopic beats ( $n=2$ ) or poor ODM signal acquisition ( $n=2$ ). In the final study population of 32 subjects, 128 pairs of measurements were obtained, and subject characteristics were mean (range) age 71 (49–86) yr, and, mean (*SD*) weight 73 (13) kg, height 167 (11) cm, and BMI 26 (6)  $\text{kg m}^{-2}$ . Twelve subjects were ASA II and 20 were ASA III. Indications for ODM monitoring were orthopaedic surgery ( $n=19$ , 59%), vascular surgery ( $n=9$ , 28%), and visceral surgery ( $n=4$ , 12%). Indications for intra-operative intervention were hypotension and CO optimization. Subjects were treated with vasopressors [phenylephrine bolus (50–100  $\mu\text{g}$ ),  $n=4$ , or norepinephrine infusion

(0.03–0.15  $\mu\text{g kg}^{-1} \text{min}^{-1}$ ),  $n=2$ ] or volume expansion ( $n=22$ ). Four subjects received both treatments.

At baseline, SAP was 102 (20) mm Hg [mean (*SD*)], DAP was 59 (13) mm Hg, MAP was 73 (14) mm Hg, and HR was 65 (13) bpm. Respiratory parameters—tidal volume/IBW: 7.9 (0.6)  $\text{ml kg}^{-1}$ ; respiratory rate 11 (2)  $\text{min}^{-1}$ ; plateau pressure 16 (4)  $\text{cm H}_2\text{O}$ ; PEEP 3 (2)  $\text{cm H}_2\text{O}$ .

As shown in Figure 1A,  $\text{CO}_{\text{ICG}}$  correlated with  $\text{CO}_{\text{ODM}}$  ( $r=0.84$ ;  $P<0.001$ ). Mean CO was 4.80 (1.87) litre  $\text{min}^{-1}$  for ICG and 4.91 (1.74) litre  $\text{min}^{-1}$  for ODM. A Bland–Altman plot (Fig. 1B) showed that the mean bias was 0.10 litre  $\text{min}^{-1}$  and the limits of agreements were  $-1.90$  litre  $\text{min}^{-1}$  and 2.11 litre  $\text{min}^{-1}$ . Percentage error was 41% according to Critchley and Critchley's method.<sup>27</sup> There was no statistically significant bias related to the following parameters: ASA score, Lee score, history of heart failure, hypertension, peripheral arterial disease, coronary syndrome, stroke, chronic kidney disease, diabetes mellitus, and smoking status. However, mean bias differed significantly when comparing COPD patients and non-COPD patients [ $-0.99$  ( $-3.43$ ; 0.26) and 0.09 ( $-1.03$ ; 2.31), respectively [values are median (min;max)];  $P<0.05$ ]. After excluding COPD patients, the Bland–Altman plot showed a mean bias of 0.47 litre  $\text{min}^{-1}$ , limits of agreements of  $-1.24$

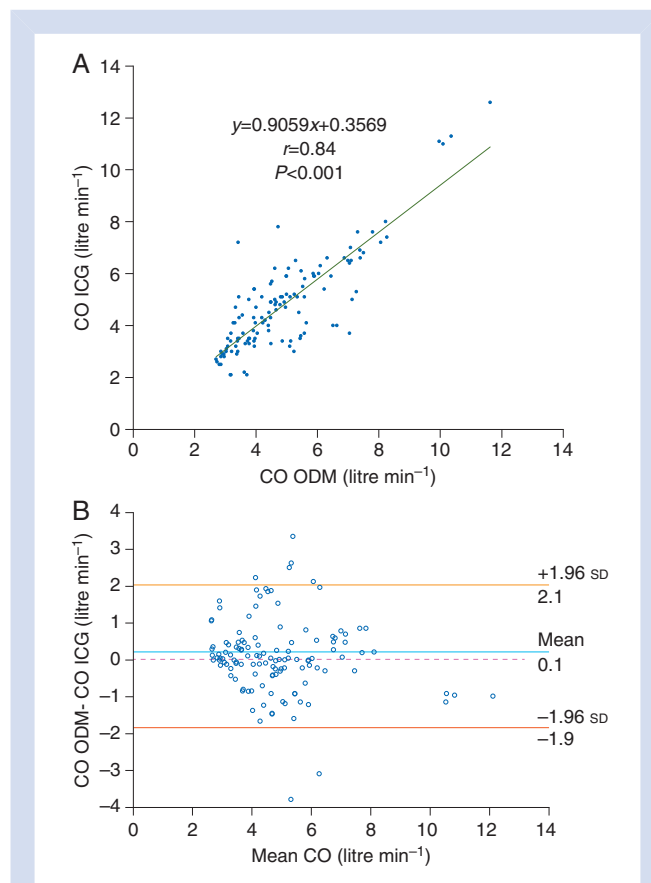


**Fig 1** (A) Pearson coefficient for the correlation between  $\text{CO}_{\text{ODM}}$  and  $\text{CO}_{\text{ICG}}$  ( $n=130$ ,  $r=0.84$ ,  $P<0.001$ ). (B) A Bland–Altman plot (mean bias: 0.10 litre  $\text{min}^{-1}$ ; limits of agreements:  $-1.90$  and 2.11 litre  $\text{min}^{-1}$ ). The percentage error was 41%.<sup>27</sup>

and 2.11 litre  $\text{min}^{-1}$ , and a percentage error of 35%. The ICG-derived LVET correlated with ODM-derived LVET ( $r=0.69$ ,  $P<0.0001$ ).

As shown in Figure 2, variations in  $\text{CO}_{\text{ICG}}$  were correlated with variations in  $\text{CO}_{\text{ODM}}$  [ $n=93$ ,  $r=0.88$  (0.82–0.94),  $P<0.0001$ ]. For four-quadrant analysis with exclusion of the central zone data (variations  $<10\%$ ), the trending ability was good [ $n=93$ , 95% confidence interval (CI) for concordance 0.86; 1.00]. After exclusion of CO variations  $<10\%$ , moderate to good trending ability was observed in a polar plot analysis (angular bias:  $-7.2^\circ$ ; 95% CI  $-12.3^\circ$ ;  $-2.5^\circ$ ), with RLAs of ( $-38^\circ$ ;  $24^\circ$ ) (Fig. 3).<sup>25</sup> For trending induced by vasopressors and fluids, the angular biases were  $-0.48^\circ$  (95% CI  $-8.72$ ; 9.67; RLA  $-23.85^\circ$ ;  $24.80^\circ$ ) and  $-9.44^\circ$  (95% CI  $-14.94^\circ$ ;  $-3.93^\circ$ ; RLA  $-38.58^\circ$ ;  $19.70^\circ$ ), respectively. As shown in Figure 4, 95% inclusion rate was obtained for a radial sector size of  $32^\circ$ , which indicates moderate to good trending ability.<sup>25</sup>

## Discussion


Four-quadrant analysis and polar plot showed that ICG trending ability was clinically acceptable relative to ODM when fluids or vasopressors were administered. After exclusion of data at the centre of the plot, the ICG–ODM concordance rate was above the value recommended by Critchley and colleagues.<sup>26</sup> The polar plot method revealed moderate to good trending and low angular bias. The advantage of the polar plot methodology over the four-quadrant plot is that the former takes account of the magnitude of the  $\Delta\text{CO}$  (rather than calculating concordance based on the direction of change only, which can create bias).<sup>26</sup> Although the changes were in the same direction, their magnitudes can differ significantly.

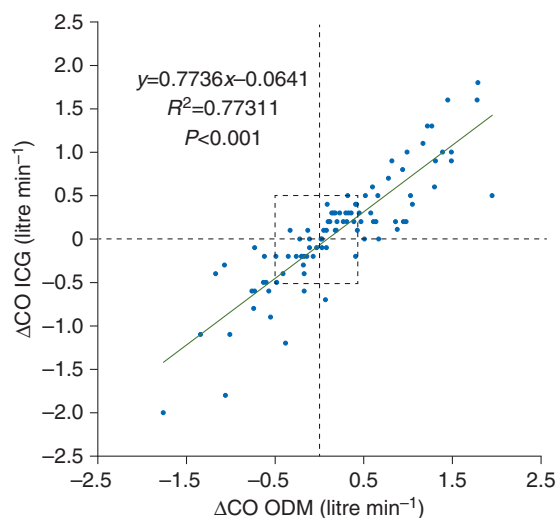


**Fig 2** Pearson coefficient for the correlation between  $\Delta\text{CO}_{\text{ODM}}$  and  $\Delta\text{CO}_{\text{ICG}}$  [ $n=93$ ,  $r=0.88$  (0.82–0.94),  $P<0.0001$ ] and a four-quadrant analysis with exclusion of central zone data ( $<0.5$  litre  $\text{min}^{-1}$ ). Good trending ability was observed in the four-quadrant plot analysis ( $n=93$ , 95% CI 0.86; 1.00).

Although a modified, repeated-measures version of the Bland–Altman method has been published,<sup>28</sup> interpretation of the limits of agreement can be complicated when repeated  $\Delta\text{CO}$  measurements from the same patient are obtained under different clinical conditions.<sup>26</sup> The RLA approach<sup>25</sup> is not valid for repeated measures, since it assumes that each data pair is independent. This would be unacceptable, as CO in a given subject will be correlated with subsequent measurements in the same individual.

Our new polar plot methodology for repeated measures has the advantage of taking into account low-magnitude  $\Delta\text{CO}$

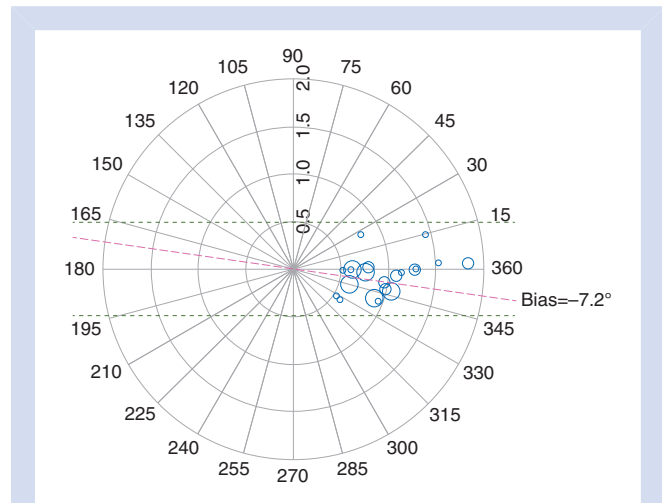

**Fig 3** Polar plot for  $\Delta\text{CO}$  values as a function of the number of  $\Delta\text{CO}$  measurements per subject (1, 2 or 3). After exclusion of CO variations  $<0.5$  litre  $\text{min}^{-1}$ , the angular bias was  $-7.2^\circ$  ( $-12.3^\circ$ ;  $-2.5^\circ$ ) and the RLA were  $-38^\circ$  and  $24^\circ$ . Measurements were recorded for  $n=22$  subjects ( $\Delta\text{CO} >0.5$  litre  $\text{min}^{-1}$ ).

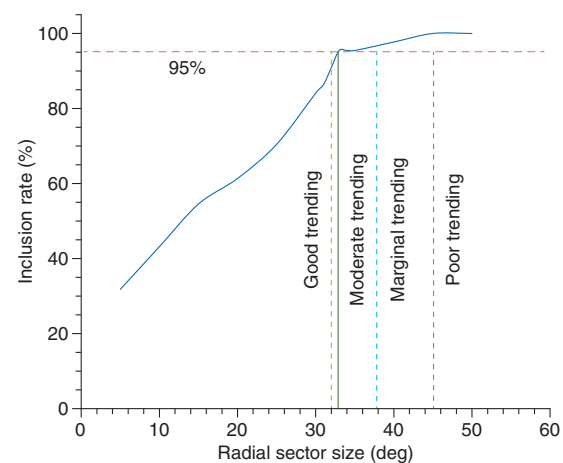

**Fig 4** Inclusion rate as a function of the radial sector size. The 95% inclusion rate was obtained for a radial sector of  $32^\circ$ , which corresponds to moderate to good trending.<sup>25</sup>

measurements that produce large polar angles. In the standard polar plot, most of the  $\Delta\text{CO}$  measurements greater than  $\pm 30^\circ$  RLA were associated with  $\Delta\text{CO}$  values between 0.59 and 0.78 litre  $\text{min}^{-1}$  with large within-subject variability. After averaging  $\Delta\text{CO}$  values, the final angle is a more accurate reflection of the concordance of  $\Delta\text{CO}$  measurements. Unlike angular bias, RLAs were broader for the new method ( $-38^\circ$ ;  $24^\circ$ ) than for the conventional method ( $-35^\circ$ ;  $22^\circ$ ), taking account of within-subject variability. This observation emphasizes that despite the conventional application of a 10% exclusion zone (0.5 litre  $\text{min}^{-1}$ ), points slightly above this cut-off point can be associated with a large angle and thus make it more difficult to assess the level of concordance. Our new method can overcome this difficulty.

We did not use a pulmonary artery catheter (PAC) as a reference for CO measurement. Monitoring with a PAC is associated with complications,<sup>29</sup> a single bolus cannot be used easily to assess trends, and new thermistor wire CO PACs are less precise<sup>30</sup> and have a long time response.<sup>31</sup> The ability of minimally invasive ODM to detect changes in CO has been demonstrated.<sup>32-34</sup> Even though the ODM device used here (CardioQ<sup>TM</sup>, Deltex Medical) measures neither instantaneous aortic diameter nor percentage split between the upper body and lower body, ODM is a minimally invasive method for CO measurement, and there is now sufficient evidence to support its use for routine cardiac monitoring.<sup>7</sup> Given that aortic diameter varies with aortic pressure, accurate measurement of SV and PV could be influenced by this variable.<sup>35</sup> Some clinical situations (shock, sepsis, laparoscopy, and epidural analgesia) modify the percentage split of flow between the upper and lower body.<sup>36-38</sup> None of our subjects experienced these events. Moreover, the clinical relevance of ODM has mainly been validated by assessing relative changes in SV in high-risk surgical patients.<sup>1-6</sup> ODM has been used to guide CO optimization with goal-directed fluid administration protocols. In these studies, researchers observed SV trends (rather than absolute values), which enhances the outcomes in high-risk surgical patients.<sup>1-6 39</sup> Hence, studying trends rather than absolute values is clinically relevant and avoids the need to estimate (i) aortic diameter and flow distribution and (ii) the geometric electrical size of the thorax.

Studies of ICG have reported conflicting results and are difficult to compare with each other because they were conducted with devices of different generations, different physical models, and different equations. The reference (comparator) method also differed from one study to another, although PAC thermodilution was most common. Subject characteristics also varied widely and ranged from healthy volunteers to patients with heart failure receiving pharmacological or surgical treatment. Two relatively dated meta-analyses<sup>40 41</sup> yielded overall correlation coefficients of 0.81 and 0.82, respectively. In a more recent meta-analysis, Peyton and Chong found that the overall correlation coefficient was 0.79 for ICG and thermodilution.<sup>9</sup> This value was similar to those for ODM (0.69), the Fick method applied to  $\text{CO}_2$  (0.57), and contour analysis of the pulse wave (0.75).<sup>9</sup> In the present study, the correlation coefficient for  $\text{CO}_{\text{ICG}}$  and

$\text{CO}_{\text{ODM}}$  was 0.84, which is similar to Peyton and Chong's value for thermodilution. In our Bland and Altman analysis, the Niccomo's<sup>TM</sup> percentage error for  $\text{CO}_{\text{ICG}}$  (41%) was out of the clinically acceptable range ( $\pm 30\%$ ). However, after excluding COPD patients ( $n=9$ ), we determined this value to be 35%. In fact, Peyton and Chong have suggested that the percentage limits of agreement for comparing two CO monitoring techniques should be raised from  $\pm 30$  to  $\pm 45\%$ .<sup>9</sup> In contrast to our present results, Fellahi and colleagues showed that the percentage error between transthoracic echocardiography and Niccomo's<sup>TM</sup>  $\text{CO}_{\text{ICG}}$  measurement was 53%.<sup>12</sup> Furthermore, there are reports of a lack of agreement between CO measured by ICG and a reference technique (usually thermodilution) in various subgroups of subjects.<sup>42-45</sup> **We observed a stronger correlation between ICG-derived LVET and Doppler-derived LVET ( $r=0.69$ ,  $P<0.000$ ) than Fellahi and colleagues ( $r=0.27$ ,  $P<0.03$ ).<sup>12</sup> This suggests that the new hardware and algorithm indeed improved the device's performance. However, disparities between our results and the literature data might also be related to the use of different reference methods.**

Several factors are known to influence ICG readings in particular clinical situations. Surgery in the area of the diaphragm or affecting the chest can decrease the accuracy of ICG, as the technique shows a poor correlation after cardiac surgery or major abdominal surgery.<sup>46</sup> Critchley and colleagues have demonstrated that abdominal opening and closure can change bias over time.<sup>47</sup> They also demonstrated (in dogs and humans) that vasodilatation/vasoconstriction status, lung fluid balance, and acute lung injury can decrease the accuracy of ICG compared with thermodilution.<sup>11 48 49</sup> The application of positive airway pressure to modify CO can also be a confounding factor that changes the thoracic volume and influences impedance measurements.<sup>12 50</sup> Indeed, we found that ICG was less accurate in patients with COPD, possibly because of differences in thoracic volume.

Our study had some other limitations. The sample size was not very large, even though the study had sufficient statistical power. We investigated a small variety of surgical procedures. The vasodilation and fluid loading treatments were not standardized but nevertheless reflected 'real life' in the operating theatre. Cost-effectiveness and outcome studies are now needed to establish whether or not the device provides clear benefits.

## Authors' contributions

E.L. and Y.M. designed the research; E.L., J.S., C.B., P.-G.G., S.P., A.K., and B.D. collected the data; E.L., Y.M., M.D., and H.D. analysed the data; M.D. performed the statistical analysis; E.L., Y.M., M.D., and H.D. wrote the paper.

## Acknowledgements

The authors thank Achille Hourdé (Imedex SARL, Jaignes, France) for providing the Niccomo monitor and electrodes.

## Declaration of interest

The authors declare that they have not received consulting fees from either Deltex Medical or Medis, or any other financial support (including departmental or institutional funding).

## Funding

The authors performed this study in the course of their normal duties as full-time employees of public-sector healthcare institutions. The electrodes and Niccom<sup>TM</sup> monitor were provided by Imedex SARL (the Medis distributor for France).

## References

- Gan TJ, Soppitt A, Maroof M, et al. Goal-directed intraoperative fluid administration reduces length of hospital stay after major surgery. *Anesthesiology* 2002; **97**: 820–6
- Conway DH, Mayall R, Abdul-Latif MS, Gilligan S, Tackaberry C. Randomised controlled trial investigating the influence of intravenous fluid titration using oesophageal Doppler monitoring during bowel surgery. *Anaesthesia* 2002; **57**: 845–9
- Wakeling HG, McFall MR, Jenkins CS, et al. Intraoperative oesophageal Doppler guided fluid management shortens postoperative hospital stay after major bowel surgery. *Br J Anaesth* 2005; **95**: 634–42
- Noblett SE, Snowden CP, Shenton BK, Horgan AF. Randomized clinical trial assessing the effect of Doppler-optimized fluid management on outcome after elective colorectal resection. *Br J Surg* 2006; **93**: 1069–76
- Sinclair S, James S, Singer M. Intraoperative intravascular volume optimisation and length of hospital stay after repair of proximal femoral fracture: randomised controlled trial. *Br Med J* 1997; **315**: 909–12
- Venn R, Steele A, Richardson P, Poloniecki J, Grounds M, Newman P. Randomized controlled trial to investigate influence of the fluid challenge on duration of hospital stay and perioperative morbidity in patients with hip fractures. *Br J Anaesth* 2002; **88**: 65–71
- NICE (National Institute for Health and Clinical Excellence). Medical technologies guidance MTG3: CardioQODM oesophageal Doppler monitor, 2011. Available from <http://guidance.nice.org.uk/MTG3/Guidance/pdf/English>
- Bernstein DP. A new stroke volume equation for thoracic electrical bioimpedance: theory and rationale. *Crit Care Med* 1986; **14**: 904–9
- Peyton PJ, Chong SW. Minimally invasive measurement of cardiac output during surgery and critical care: a meta-analysis of accuracy and precision. *Anesthesiology* 2010; **113**: 1220–35
- Bernstein DP, Lemmens HJ, Brodsky JB. Limitations of impedance cardiography. *Obes Surg* 2005; **15**: 659–60
- Critchley LA, Calcroft RM, Tan PY, Kew J, Critchley JA. The effect of lung injury and excessive lung fluid, on impedance cardiac output measurements, in the critically ill. *Intensive Care Med* 2000; **26**: 679–85
- Fellahi JL, Caille V, Charron C, Deschamps-Berger PH, Vieillard-Baron A. Noninvasive assessment of cardiac index in healthy volunteers: a comparison between thoracic impedance cardiography and Doppler echocardiography. *Anesth Analg* 2009; **108**: 1553–9
- Keren H, Burkhoff D, Squara P. Evaluation of a noninvasive continuous cardiac output monitoring system based on thoracic bioimpedance. *Am J Physiol Heart Circ Physiol* 2007; **293**: H583–9
- Raval NY, Squara P, Cleman M, Yalamanchili K, Winklmaier M, Burkhoff D. Multicenter evaluation of noninvasive cardiac output measurement by bioimpedance technique. *J Clin Monit Comput* 2008; **22**: 113–9
- Fagnoul D, Vincent JL, Backer DD. Cardiac output measurements using the bioimpedance technique in critically ill patients. *Crit Care* 2012; **16**: 460
- Kober D, Trepte C, Petzoldt M, et al. Cardiac index assessment using bioimpedance in patients undergoing cytoreductive surgery in ovarian carcinoma. *J Clin Monit Comput* 2013; **27**: 621–7
- Kupersztych-Hagege E, Teboul JL, Artigas A, et al. Bioimpedance is not reliable for estimating cardiac output and the effects of passive leg raising in critically ill patients. *Br J Anaesth* 2013; **111**: 961–6
- Aroom KR, Harting MT, Cox CS Jr, Radharkrishnan RS, Smith C, Gill BS. Bioimpedance analysis: a guide to simple design and implementation. *J Surg Res* 2009; **153**: 23–30
- Lababidi Z, Ehmke DA, Durnin RE, Leaverton PE, Lauer RM. The first derivative thoracic impedance cardiogram. *Circulation* 1970; **41**: 651–8
- Singer M, Bennett ED. Noninvasive optimization of left ventricular filling using esophageal Doppler. *Crit Care Med* 1991; **19**: 1132–7
- Bernardin G, Tiger F, Fouche R, Mattei M. Continuous noninvasive measurement of aortic blood flow in critically ill patients with a new esophageal echo-Doppler system. *J Crit Care* 1998; **13**: 177–83
- Guinot PG, de Broca B, Abou Arab O, et al. Ability of stroke volume variation measured by oesophageal Doppler monitoring to predict fluid responsiveness during surgery. *Br J Anaesth* 2013; **110**: 28–33
- Mahjoub Y, Touzeau J, Airapetian N, et al. The passive leg-raising maneuver cannot accurately predict fluid responsiveness in patients with intra-abdominal hypertension. *Crit Care Med* 2010; **38**: 1824–9
- Fosgate GT. Practical sample size calculations for surveillance and diagnostic investigations. *J Vet Diagn Invest* 2009; **21**: 3–14
- Critchley LA, Yang XX, Lee A. Assessment of trending ability of cardiac output monitors by polar plot methodology. *J Cardiothorac Vasc Anesth* 2011; **25**: 536–46
- Critchley LA, Lee A, Ho AM. A critical review of the ability of continuous cardiac output monitors to measure trends in cardiac output. *Anesth Analg* 2010; **111**: 1180–92
- Critchley LA, Critchley JA. A meta-analysis of studies using bias and precision statistics to compare cardiac output measurement techniques. *J Clin Monit Comput* 1999; **15**: 85–91
- Myles PS, Cui J. Using the Bland–Altman method to measure agreement with repeated measures. *Br J Anaesth* 2007; **99**: 309–11
- National Heart, Lung, and Blood Institute Acute Respiratory Distress Syndrome (ARDS) Clinical Trials Network, Wheeler AP, Bernard GR, et al. Pulmonary-artery versus central venous catheter to guide treatment of acute lung injury. *N Engl J Med* 2006; **354**: 2213–24
- Zollner C, Goetz AE, Weis M, et al. Continuous cardiac output measurements do not agree with conventional bolus thermodilution cardiac output determination. *Can J Anaesth* 2001; **48**: 1143–7
- Mihm FG, Gettinger A, Hanson CW III, et al. A multicenter evaluation of a new continuous cardiac output pulmonary artery catheter system. *Crit Care Med* 1998; **26**: 1346–50
- Valtier B, Cholley BP, Belot JP, de la Coussaye JE, Mateo J, Payen DM. Noninvasive monitoring of cardiac output in critically ill patients using transesophageal Doppler. *Am J Respir Crit Care Med* 1998; **158**: 77–83
- Roeck M, Jakob SM, Boehlen T, Brander L, Knuesel R, Takala J. Change in stroke volume in response to fluid challenge: assessment using esophageal Doppler. *Intensive Care Med* 2003; **29**: 1729–35

- 34 Kim K, Kwok I, Chang H, Han T. Comparison of cardiac outputs of major burn patients undergoing extensive early escharectomy: esophageal Doppler monitor versus thermodilution pulmonary artery catheter. *J Trauma* 2004; **57**: 1013–7
- 35 Monnet X, Rienzo M, Osman D, et al. Esophageal Doppler monitoring predicts fluid responsiveness in critically ill ventilated patients. *Intensive Care Med* 2005; **31**: 1195–201
- 36 Schober P, Loer SA, Schwarte LA. Perioperative hemodynamic monitoring with transesophageal Doppler technology. *Anesth Analg* 2009; **109**: 340–53
- 37 Leather HA, Wouters PF. Oesophageal Doppler monitoring overestimates cardiac output during lumbar epidural anaesthesia. *Br J Anaesth* 2001; **86**: 794–7
- 38 Cariou A, Monchi M, Joly LM, et al. Noninvasive cardiac output monitoring by aortic blood flow determination: evaluation of the Sometec Dynemo-3000 system. *Crit Care Med* 1998; **26**: 2066–72
- 39 Chytra I, Pradl R, Bosman R, Pelnar P, Kasal E, Zidkova A. Esophageal Doppler-guided fluid management decreases blood lactate levels in multiple-trauma patients: a randomized controlled trial. *Crit Care* 2007; **11**: R24
- 40 Fuller HD. The validity of cardiac output measurement by thoracic impedance: a meta-analysis. *Clin Invest Med* 1992; **15**: 103–12
- 41 Raaijmakers E, Faes TJ, Scholten RJ, Goovaerts HG, Heethaar RM. A meta-analysis of three decades of validating thoracic impedance cardiography. *Crit Care Med* 1999; **27**: 1203–13
- 42 Doering L, Lum E, Dracup K, Friedman A. Predictors of between-method differences in cardiac output measurement using thoracic electrical bioimpedance and thermodilution. *Crit Care Med* 1995; **23**: 1667–73
- 43 Genoni M, Pelosi P, Romand JA, Pedoto A, Moccetti T, Malacrida R. Determination of cardiac output during mechanical ventilation by electrical bioimpedance or thermodilution in patients with acute lung injury: effects of positive end-expiratory pressure. *Crit Care Med* 1998; **26**: 1441–5
- 44 Marik PE, Pendelton JE, Smith R. A comparison of hemodynamic parameters derived from transthoracic electrical bioimpedance with those parameters obtained by thermodilution and ventricular angiography. *Crit Care Med* 1997; **25**: 1545–50
- 45 Young JD, McQuillan P. Comparison of thoracic electrical bioimpedance and thermodilution for the measurement of cardiac index in patients with severe sepsis. *Br J Anaesth* 1993; **70**: 58–62
- 46 Fellahi JL, Fischer MO, Rebet O, Massetti M, Gerard JL, Hanouz JL. A comparison of endotracheal bioimpedance cardiography and transpulmonary thermodilution in cardiac surgery patients. *J Cardiothorac Vasc Anesth* 2012; **26**: 217–22
- 47 Critchley LA, Leung DH, Short TG. Abdominal surgery alters the calibration of bioimpedance cardiac output measurement. *Int J Clin Monit Comput* 1996; **13**: 1–8
- 48 Critchley LA, Peng ZY, Fok BS, James AE. The effect of peripheral resistance on impedance cardiography measurements in the anesthetized dog. *Anesth Analg* 2005; **100**: 1708–12
- 49 Peng ZY, Critchley LA, Fok BS. An investigation to show the effect of lung fluid on impedance cardiac output in the anaesthetized dog. *Br J Anaesth* 2005; **95**: 458–64
- 50 Bikker IG, Preis C, Egal M, Bakker J, Gommers D. Electrical impedance tomography measured at two thoracic levels can visualize the ventilation distribution changes at the bedside during a decremental positive end-expiratory lung pressure trial. *Crit Care* 2011; **15**: R193
- 51 Laird NM, Ware JH. Random-effects models for longitudinal data. *Biometrics* 1982; **38**: 963–74
- 52 Bland JM, Altman DG. Measuring agreement in method comparison studies. *Stat Methods Med Res* 1999; **8**: 135–60
- 53 Efron B. Bootstrap methods: another look at the jackknife. *Ann Statist* 1979; **7**: 1–26

## Appendix: the polar plot method for repeated measures

The modified Bland–Altman method for repeated measures can be used to calculate the mean of repeated measures for each method and for each individual. The mean angles for each subject can then be used to compare the two methods (based on an RLA of  $\pm 30^\circ$ ). The bias between the two methods is not affected by averaging the repeated measures. However, the variation in the differences between original measurements is underestimated by this practice because the measurement error is, to a certain extent, eliminated. Advanced statistical calculation is therefore necessary to take these measurement errors into account.

A random effects model was used to estimate within-subject variation after accounting for other observed variations,<sup>51</sup> in which each subject presented a different bias, magnitude, and angle over the observation period. An appropriate polar plot for repeated measures was created on the basis of within-subject variance estimated from the random effects model. According to the Bland–Altman method,<sup>52</sup> the SD of the angles of the repeated measures can be calculated from within-subject SD estimates. The random effect is the sequence or the measurement time over the observation period.

We also developed a new presentation of the polar plot by using the average  $\Delta$ CO measurements for each subject. Each subject is represented once (by a circle) in the plot. The diameter of the circle is proportional to the number of measurements recorded for that subject. To assess RLA with this method, components of the variance for the polar angle were estimated in a mixed-model analysis of variance. To evaluate uncertainty in the estimated parameter (concordance rate and angular bias), 1000 bootstrap replications<sup>53</sup> were carried out and 95% percentile-based confidence intervals were established. Using a conservative approach, the lower confidence limit for the RLA was defined as the 2.5% percentile of 1000-bootstrap lower limits of agreement and the upper confidence limit was defined as the 97.5% percentile of 1000-bootstrap lower limits of agreement.

Handling editor: H. C. Hemmings